

BATINGA ANIMAL MEDICAL CENTER
Nucleic Acid Test Report



Pet Name: MILO
Gender: Male
Sample No.:
Test Item: CPI(CPV)

Owner Tel.:
Species: Canine
Test Time: 2026-06-12 13:41

Owner Name: ACANG
Pet Age: 1 Month
Patient Number:

Test Results

Test Item	CT	Reference	Result
CPV	32.8	>36.0 Or NoCt	Positive(+)
IC	17.8	>38.0 Or NoCt	Positive(+)

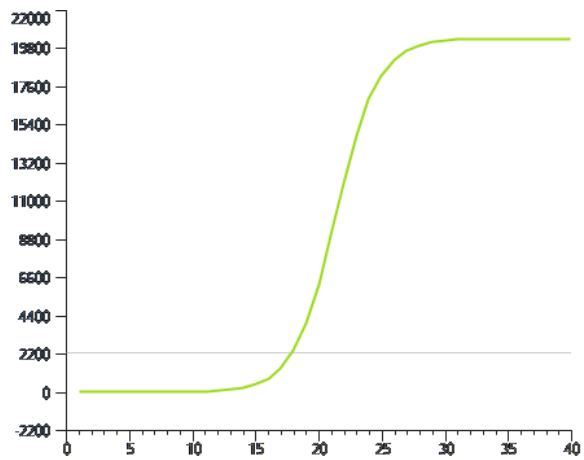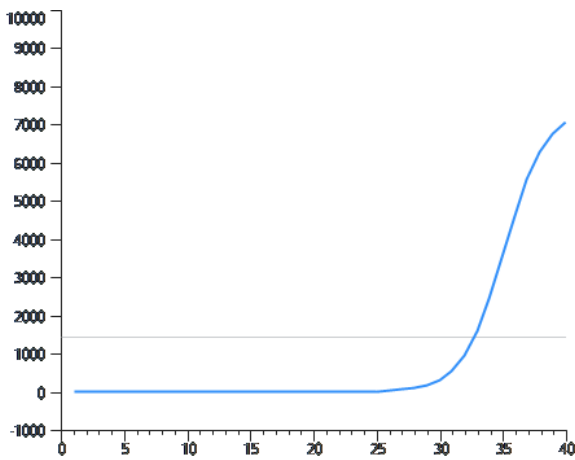

Result Interpretation:

1. Positive Result (+): The current test sample contains the target substance (pathogen or internal control);
2. Negative Result (-): The target substance (pathogen or internal standard) in the current test sample is either below the detection limit or absent;
3. CT > Ref. Range, suggests infection window or recovery phase. Clinical correlation required. Recommend retesting within 24-48 hours to monitor CT dynamics;
4. CT Number Reference Interval: Reference interval used to distinguish the presence or absence of the target substance based on CT numbers.If CT > 30, the viral load is low, and the risk of transmission is low, indicating that the animal may be asymptomatic or in a subclinical state.

Note: The test results are only valid for the samples submitted this time and are for clinical reference only.

Testing Physician:

Chief Physician:

Hospital Tel.: 09061211260

Report Date: 2026-06-12

Hospital Addc: SM CITY CDO UPTOWN, MASTERSONS AVE., CARMEN, CAGAYAN DE ORO

